


Pall Breathing System Filters Stop SARS-CoV-2

The SARS-CoV-2 pandemic has affected many people, including health care workers and claimed the lives of more than 3 million.


Pall Breathing System Filters (Ultipor® 25, Ultipor® 50, Ultipor® 100 and BB50TE) have been shown in laboratory testing to retain aerosolized SARS-CoV-2 viruses at > 99.999 % efficiency¹

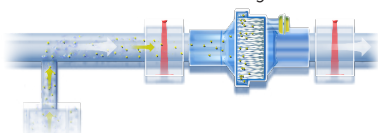

Clinical studies have previously shown that Pall Breathing System Filters meet the highest performance standards in the prevention of cross contamination^{2,3}



We can confirm:

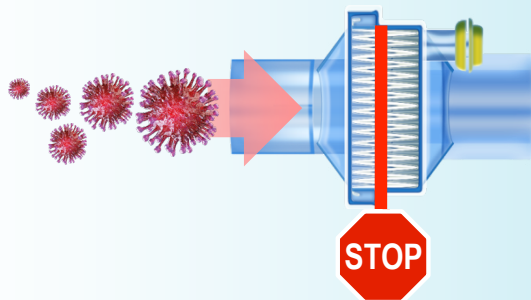

Pall Breathing System Filters have been shown to retain > 99.999 % of the aerosolized SARS-CoV-2 and are expected to form an effective barrier against airborne virus contamination from ventilated patient's exhaled breath⁴

¹ Pall SLS Technical Reports 2021 - This claim has been cleared for Europe under CE mark. It has not been cleared by the FDA

² Hübner et al. (2011); GMS Krankenhaushygiene Interdisziplinär Vol. 6(1) ISSN 18635245

³ Dubler et al. (2016); Acta Anaesthesiologica Scandinavica Oct;60(9):1251-60

⁴ Leung NH, Chu DK, Shiu EY, et al. Respiratory virus shedding in exhaled breath and efficacy of face masks (Nat Med. 2020;26:676-680